

## Can We Detect Carotid Artery Stenosis From Skin Vibrations: A Computational Investigation of High-Frequent Flow Under Physiological Varying Flow Conditions.

Viviana Mancini<sup>1</sup>, Aslak Bergersen<sup>2</sup>, Jan Vierendeels<sup>3</sup>, Patrick Segers<sup>1</sup>, Kristian Valen-Sendstad<sup>2</sup>

<sup>1</sup>Ghent University, bioMMeda, Ghent, Belgium. <sup>2</sup>Simula Research Laboratory, Computational Cardiac Modelling, Lysaker, Norway. <sup>3</sup>Ghent University, Department of Flow, heat and combustion mechanics, Ghent, Belgium.

### Abstract

#### Introduction

Carotid artery stenoses are a major cause of stroke with a prevalence of 4.2% in the population<sup>1</sup> and are often asymptomatic. Therefore, it is a need for a quick and portable screening method. A newly suggested method for screening is using a laser Doppler vibrometer, which can detect skin vibrations induced by a high-frequent post-stenotic flow. However, we do not know if all stenoses harbor such instabilities. The aim of this study was to investigate how high-frequent flow instabilities vary with the degree of stenosis, inlet flow rate, and outlet flow split.

#### Methods

A computed tomography image of a 76 % stenosed internal carotid artery (ICA) was segmented and then altered to obtain models ranging from a mild stenosis to almost complete occlusion: 56%, 66%, 86%, and 96%, as illustrated in Fig1A. The inlet flow rates, with a physiologically plausible waveform<sup>2</sup>, and outflow splits were varied with mean plus/minus one and two standard deviations<sup>3,4</sup>, respectively, see Fig1C-D. Furthermore, since flow rates and splits vary with the degree of stenosis, we also changed these alongside with the degree of stenosis, see Fig1B. We assumed blood to behave as a Newtonian fluid with kinematic viscosity  $\nu=3.3 \cdot 10^{-6} \text{m}^2/\text{s}$  and used our kinetic energy preserving and minimally dissipative, second order solver *Oasis*<sup>5</sup> to simulate for two cardiac cycles and reported the velocity magnitude from the latter measured in point P, see Fig1A. We used 20.000 time steps per cycle and meshes with ~15 million linear elements, resulting in an average cell length of  $\Delta x_{\text{mean}}=1.92 \cdot 10^{-4} \text{m}$ .

#### Results

Fig1E shows the qualitative results from varying the degree of stenosis, and we can observe that the models with a stenosis severity less than 70 % harbored high-frequent fluctuations. Fig1F-G shows the results from varying the flow rate and split, respectively, and both exhibited similar trends; increased ICA flow rate enlarged the fluctuations.

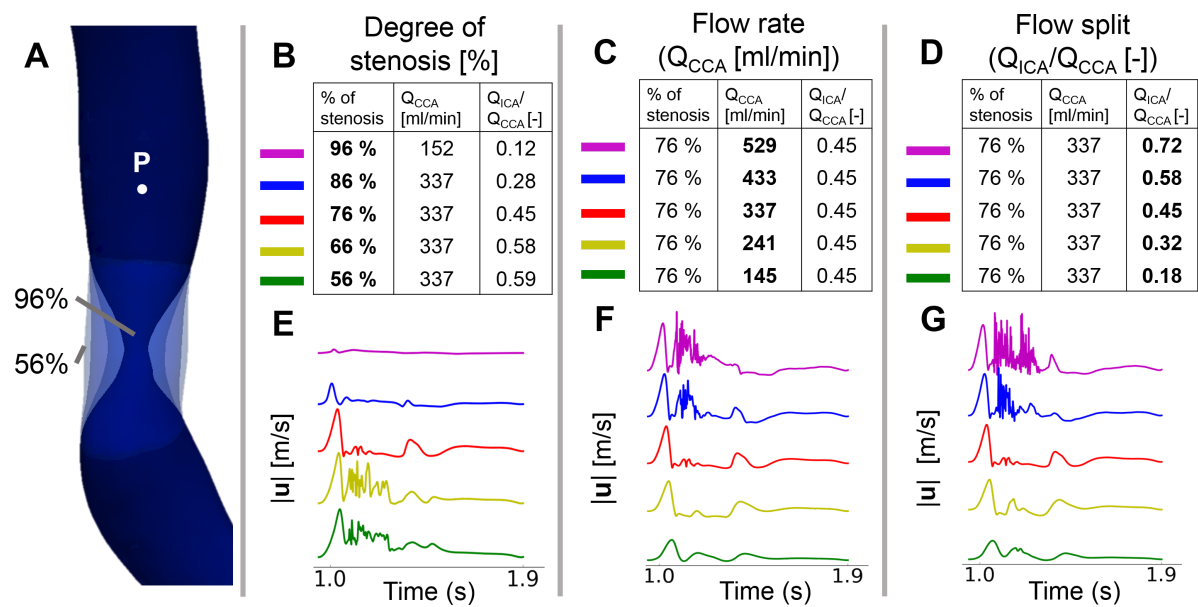


Fig1 **A**: Variable degree of stenoses in the internal carotid artery, and a point P located 1 diameter downstream of the stenosis. **B**, **C**, and **D**: List of simulations, with varying degree of stenosis, flow rate, and flow split, respectively. **E**, **F**, and **G**: Velocity magnitude ( $|u|$ ) in point P of the corresponding list simulations in **B**, **C**, and **D**, respectively.

Discussion

We only observed fluctuations in moderate ( $< 70\%$ ) stenosis models, which can physiologically be explained by a reduction in flow rate due to an increased pressure drop over the stenosis. If the simulated results reflect physiology, and not modeling assumptions, the LDV is promising for detecting early-stage carotid artery stenosis. In future work, we will investigate flow fluctuations in healthy subjects to understand the risk of false positives.

Acknowledgments

Funded by H2020 ICT-26-2014 CARDIS.

References

1. de Weerd M et al., *Stroke* **40**,1105–1113 (2009).
2. Hoi Y et al., *Physiol. Meas.* **31**,291-302 (2010).
3. Groen HC et al., *J. Biomech.* **43**, 2332–2338 (2010).
4. Likittanasombut P et al., *J. Neuroimaging* **16**,34–38 (2006).
5. Mortensen M & Valen-Sendstad K, *Comput. Phys. Commun.* (2016).